

[www.costeffectiveequipment.com](http://www.costeffectiveequipment.com)

+1-573-466-4300

# Operations Manual

Apogee® 300 Bake Plate

Model: A-B-B3-2



  
Cost Effective Equipment

<b>1</b>	<b>INTRODUCTION.....</b>	<b>4</b>
1.1	CONFIDENTIALITY STATEMENT .....	4
1.2	WARRANTY .....	4
1.3	RETURNED MATERIALS .....	4
1.4	MODEL AND REVISIONS .....	4
1.5	ENVIRONMENTAL CONSIDERATIONS .....	5
1.6	GENERAL SAFETY HAZARDS / PRECAUTIONS .....	5
1.7	ELECTRICAL .....	6
1.8	MECHANICAL.....	6
1.9	THERMAL.....	6
1.10	CHEMICAL.....	6
1.11	LOCKOUT/TAGOUT PROCEDURES AND INFORMATION.....	7
1.12	INTENDED USE OF MACHINE.....	8
<b>2</b>	<b>EQUIPMENT DESCRIPTION .....</b>	<b>9</b>
2.1	USER CONTROLS .....	9
2.2	DIMENSIONS .....	9
2.3	FEATURES & PROGRAMMABILITY.....	10
2.4	PRECISION.....	10
2.5	RELIABILITY .....	10
2.6	NRTL .....	10
2.7	UTILITIES .....	11
<b>3</b>	<b>INSTALLATION.....</b>	<b>12</b>
3.1	CLEARANCE REQUIREMENTS .....	12
3.2	FACILITIES REQUIREMENTS .....	13
3.3	ENVIRONMENT .....	14
3.4	UNPACKAGING & INSPECTION.....	14
3.5	SYSTEM INSTALLATION & SETUP.....	14
3.6	START UP .....	15
3.7	SYSTEM CHECKS.....	15
<b>4</b>	<b>DATASTREAM™ TECHNOLOGY .....</b>	<b>18</b>
4.1	SYSTEM PARAMETERS .....	18
4.2	MANUAL CONTROLS – APOGEE® 300 BAKE PLATE.....	18
4.3	PREPARATION .....	23
4.4	RUNNING RECIPES .....	24
4.5	EDITING RECIPES .....	25
4.6	TOOL SPECIFIC SETTINGS – APOGEE® 300 BAKE PLATE .....	26
<b>5</b>	<b>BAKE PLATE THEORY .....</b>	<b>27</b>
5.1	BAKE PLATES VS CONVENTIONAL OVENS .....	27
5.2	THE SKIN EFFECT .....	27
5.3	HOTPLATE BAKE VARIABLES AND METHODS .....	28
5.4	BAKE TEMPERATURE .....	28
5.5	BAKE METHODS.....	28
5.6	BAKE TIME.....	29
5.7	EXHAUST COVER .....	29
5.8	OVEN VS BAKE PLATE EXAMPLES .....	29
5.9	REFLOW SOLDERING .....	30
5.10	BAKE PLATE PROCESS TROUBLESHOOTING.....	30

**6    PREVENTATIVE MAINTENANCE .....31**

6.1    SERVICE AND REPAIRS .....31

6.2    FAULT CONDITION .....31

6.3    SAFETY CHECKS .....31

6.4    MECHANICAL/UTILITIES CHECKLIST .....31

6.5    CLEANING .....32

**7    TABLE OF REVISIONS .....33**

1 **Introduction**

1.1 **Confidentiality Statement**

Information supplied is for the use in the operation and/or maintenance of Cee® equipment. Neither this document nor the information it contains shall be disclosed to others for manufacturing or any other purpose without written authorization from Cost Effective Equipment, LLC.

1.2 **Warranty**

Cost Effective Equipment, LLC warrants to the original purchaser (Buyer) that equipment is free from defects in material and workmanship under normal use and service in accordance with Cee® instructions and specifications. Buyer shall promptly notify Cee® of any claim against this warranty, and any item to be returned to Cee® shall be sent with transportation charges prepaid by Buyer, clearly marked with a Return Authorization (RMA) number obtained from Cee® Customer Support. Cee’s obligation under this warranty is limited to the repair or replacement, at Cee’s option, of any equipment, component or part which is determined by Cee® to be defective in material or workmanship. This obligation shall expire one (1) year after the initial shipment of the equipment from Cee®. This warranty shall be void if:

- Any failure is due to the misuse, neglect, improper installation of, or accident to the equipment.
- Any major repairs or alterations are made to equipment by anyone other than a duly authorized representative of Cee®. Representatives of Buyer will be authorized to make repairs to the equipment without voiding warranty, on completion of the Cee® training program.
- Replacement parts are used other than those made or recommended by Cee®.

CEE® MAKES NO OTHER WARRANTIES, EXPRESSED OR IMPLIED, WITH RESPECT TO EQUIPMENT. NO WARRANTY IS MADE AS TO THE MERCHANTABILITY OF THE EQUIPMENT NOR ITS FITNESS FOR ANY PARTICULAR PURPOSE. In no event shall Cee® be liable for consequential loss or damages, however caused. No person or representative of Cee® is authorized to assume for Cee® any liability in connection with equipment nor to make any change to this warranty unless such change or modification is put in writing and approved by an authorized representative of Cee® in writing.

This warranty shall be governed by the laws of the state of Missouri, U.S.A.

1.3 **Returned Materials**

Any materials, parts, or equipment returned to Cost Effective Equipment, LLC must be clearly labeled with a Return Material Authorization (RMA) number.




To obtain an RMA number, contact:

Cost Effective Equipment, LLC Customer Support  
Telephone .....+1-573-466-4300  
Email.....[support@costeffectiveequipment.com](mailto:support@costeffectiveequipment.com)  
Web Address.....[www.costeffectiveequipment.com](http://www.costeffectiveequipment.com)  
Physical Address.....6 Industrial Drive; St. James, Missouri 65559




1.4 **Model and Revisions**

The model and serial number information for the Cee® Apogee® 300 Bake Plate are located on the rear panel. Software version information can be found on the *About* screen. Refer to the [\*DataStream™ Manual\*](#) for screen shots and a detailed explanation of the system software.




## 1.5 Environmental Considerations

	Cee® fosters sustainability through innovation in the durability and reliability of our precision tools and equipment. Individual component modules are engineered for serviceability ensuring long lasting performance. Processes are designed to minimize use & consumption of chemical compounds ensuring accurate, replicable, industry-leading results every time.	Cee® favorise la durabilité grâce à l'innovation dans la durabilité et la fiabilité de nos outils et équipements de précision. Les modules de composants individuels sont conçus pour une facilité d'entretien garantissant des performances durables. Les processus sont conçus pour minimiser l'utilisation et la consommation de composés chimiques, garantissant à chaque fois des résultats précis, reproductibles et à la pointe de l'industrie.
	Cee® diligently screens suppliers to ensure conflict-free sourcing of minerals and product components are constructed of recycled materials wherever possible.	Cee® sélectionne avec diligence les fournisseurs pour garantir que l'approvisionnement en minéraux est sans conflit et que les composants des produits sont fabriqués à partir de matériaux recyclés dans la mesure du possible.
	Cee® tools and equipment operate without the use of ozone depleting substances (ODSs) including chlorofluorocarbons (CFCs), methyl chloroform, hydrochlorofluorocarbons (HCFCs), carbon tetrachloride, perfluoro compounds (PFCs), or other volatile compounds/organic solvents.	Les outils et équipements Cee® fonctionnent sans utilisation de substances appauvrissant la couche d'ozone (SACO), notamment les chlorofluorocarbures (CFC), le méthyle chloroforme, les hydrochlorofluorocarbures (HCFC), le tétrachlorure de carbone, les composés perfluorés (PFC) ou d'autres composés volatils/solvants organiques.




## 1.6 General Safety Hazards / Precautions

	Read this manual in its entirety before operating or servicing the machine.	Lisez ce manuel dans son intégralité avant d'utiliser ou d'entretenir la machine.
	The unit is very heavy and proper precautions should be taken when handling the machine to minimize the risk of injury. Labels are placed on the machine to identify areas where caution is needed during operation.	L'unité est très lourde et des précautions appropriées doivent être prises lors de la manipulation de la machine pour minimiser le risque de blessure. Des étiquettes sont placées sur la machine pour identifier les zones où des précautions sont nécessaires pendant le fonctionnement.
	Sound pressure measurements greater than 80dB(A) are considered hazardous. The following sound pressure measurements were obtained from the Cee® Apogee® 300 Bake Plate at a distance of 3 ft (0.9 m) from the system:  Stand-by Mode: 40dB(A) Normal Operations: 40dB(A)	Les mesures de pression acoustique supérieures à 80 dB(A) sont considérées comme dangereuses. Les mesures de pression acoustique suivantes ont été obtenues à partir de la plaque de cuisson Cee® Apogee® 300 à une distance de 3 pieds (0,9 m) du système:  Mode veille: 40 dB(A) Fonctionnement normal: 40 dB(A)


## 1.7 Electrical

	High voltage is present in the machine. Disconnect power before servicing.	Une haute tension est présente dans la machine. Débranchez l'alimentation avant l'entretien.
	Stored electrical energy is present in the machine. Before servicing allow sufficient time for discharge.	L'énergie électrique stockée est présente dans la machine. Avant l'entretien, prévoyez suffisamment de temps pour la décharge.
	This unit must be connected to an outlet with proper grounding.	Cet appareil doit être connecté à une prise avec une mise à la terre appropriée.

## 1.8 Mechanical

	This machine may contain compressed gases which can provide motive force for components and can expand violently upon decompression. Disconnect N2 or CDA before removing any panels.	Cette machine peut contenir des gaz comprimés qui peuvent fournir une force motrice aux composants et peuvent se dilater violemment lors de la décompression. Débranchez le N2 ou le CDA avant de retirer les panneaux.
	Ensure that all panels are on and in their correct locations before powering up or operating.	Assurez-vous que tous les panneaux sont allumés et à leur emplacement correct avant la mise sous tension ou l'utilisation.
	When opening lids be aware of the pinch point at the hinge cover. Open lids only by using the handles on the lids.	Lorsque vous ouvrez les couvercles, faites attention au point de pincement au niveau du cache de la charnière. Ouvrez les couvercles uniquement en utilisant les poignées des couvercles.

## 1.9 Thermal

	Bake Plates can reach temperatures sufficient to cause severe burns and may remain hot for a long-time following operation. Do not service the machine until all surfaces have cooled to a safe thermal condition (e.g., room temperature).	Les plaques de cuisson peuvent atteindre des températures suffisantes pour provoquer de graves brûlures et peuvent rester chaudes longtemps après l'opération. N'entretenez pas la machine tant que toutes les surfaces n'ont pas refroidi à un état thermique sûr (par exemple, température ambiante).
---	---	---

## 1.10 Chemical

Cee® does not supply or dictate chemicals to be used in conjunction with the Cee® Apogee® 300 Bake Plate. Material data will be reviewed during equipment design and configuration to ensure compatibility with the customer's proprietary process.

Cee® ne fournit ni n'impose aucun produit chimique à utiliser avec la plaque de cuisson Cee® Apogee® 300. Les données matérielles seront examinées lors de la conception et de la configuration de l'équipement pour garantir la compatibilité avec le processus exclusif du client.

<p>Prior to introducing new chemicals, refer to your chemical supplier's factory specifications and MSDS. Material Safety Data Sheets (MSDS) contain crucial information regarding chemical safety, including details about hazardous components, physical properties, spill and leak procedures, waste disposal guidelines, and personal protective equipment requirements for handling.</p>		<p>Avant d'introduire de nouveaux produits chimiques, reportez-vous aux spécifications d'usine et à la fiche signalétique de votre fournisseur de produits chimiques. Les fiches signalétiques (MSDS) contiennent des informations cruciales concernant la sécurité chimique, notamment des détails sur les composants dangereux, les propriétés physiques, les procédures en cas de déversement et de fuite, les directives d'élimination des déchets et les exigences en matière d'équipement de protection individuelle pour la manipulation.</p>
	<p>Ensure chemical compatibility of all chemicals and materials being used inside the machine. This includes all wetted parts of the storage, supply, dispense, and waste systems.</p>	<p>Assurer la compatibilité chimique de tous les produits chimiques et matériaux utilisés à l'intérieur de la machine. Cela inclut toutes les parties mouillées des systèmes de stockage, d'alimentation, de distribution et de déchets.</p>
	<p>Potential for flammable Chemicals. No open flames/sparks.</p>	<p>Potentiel de produits chimiques inflammables. Pas de flammes nues/étincelles.</p>
	<p>Relieve pressure and shut off chemical valves before servicing supply lines, dispense valves or other components.</p>	<p>Relâchez la pression et fermez les vannes chimiques avant d'entretenir les conduites d'alimentation, les vannes de distribution ou d'autres composants.</p>
	<p>Ensure proper ventilation/exhaust is always used.</p>	<p>Assurez-vous qu'une ventilation/évacuation adéquate est toujours utilisée.</p>
	<p>Always wear appropriate Personal Protective Equipment. This includes safety glasses, gloves, and other equipment, as needed, to protect from mechanical and chemical hazards.</p>	<p>Portez toujours un équipement de protection individuelle approprié. Cela comprend des lunettes de sécurité, des gants et tout autre équipement, si nécessaire, pour se protéger des risques mécaniques et chimiques.</p>
<p>Exhaust and fume management is important to prevent the release of hazardous materials and ensure a safe working environment. Users should assume that all fumes are hazardous and take appropriate precautions to ensure system exhaust is functional per the guidelines outlined in section 6 of this manual.</p>		<p>La gestion des gaz d'échappement et des fumées est importante pour empêcher le rejet de matières dangereuses et garantir un environnement de travail sûr. Les utilisateurs doivent supposer que toutes les fumées sont dangereuses et prendre les précautions appropriées pour garantir que l'échappement du système est fonctionnel conformément aux directives décrites dans la section 6 de ce manuel.</p>

### 1.11 Lockout/Tagout Procedures and Information

Before servicing, turn off the machine and remove the power inlet cord by disconnecting the plug where it enters the machine.

**Note:** There are no LOTO (Lock Out/Tag Out) facilities supplied with the Cee® Apogee® 300 Bake Plate. It is the responsibility of the customer/installer/end-user to ensure that the suitable LOTO devices are provided on utilities being supplied to the Cee® Apogee® 300 Bake Plate in accordance with applicable laws, regulations, and/or company policies.

For more information, please contact [Cee® Customer Support](#).

## 1.12 Intended Use of Machine

The Cee® Apogee® 300 Bake Plate is intended for use as a semiconductor/optical application machine.

The Cee® Apogee® 300 Bake Plate is not intended for use in food or medical applications or for use in hazardous locations.

The Cee® Apogee® 300 Bake Plate is intended for use only by trained personnel wearing the proper personal protective equipment. Anyone not trained in the proper use of the Cee® Apogee® 300 Bake Plate and having not fully read this manual, should not operate the equipment.

The Cee® Apogee® 300 Bake Plate is intended for use in a cleanroom environment to provide the proper processing conditions for substrates. If it is used outside of a cleanroom environment, substrate cleanliness may be compromised.

The Cee® Apogee® 300 Bake Plate is not intended for use in a hazardous or explosive environment.

### **Normal Operating Conditions**

The Cee® Apogee® 300 Bake Plate is designed for indoor use only.

Ambient Temperature ..... 10°C - 30°C

Relative Humidity ..... ≤80%

Altitude ..... up to 3000 m

Pollution Degree..... 2

Overvoltage Category ..... II

Permissible Voltage Fluctuations ..... 208-230VAC ±10%



If the Cee® Apogee® 300 Bake Plate is used in a manner not specified by Cee® or with accessories not provided by Cee® the protection provided by the equipment may be impaired.

Si la plaque de cuisson Cee® Apogee® 300 est utilisée d'une manière non spécifiée par Cee® ou avec des accessoires non fournis par Cee®, la protection fournie par l'équipement peut être altérée.



## 2 Equipment Description

The Cee® Apogee® 300 Bake Plate features a revolutionary intuitive interface, a space-saving design, and track-quality thermal accuracy and uniformity.

Fully programmable and user-friendly, the Cee® Apogee® 300 Bake Plate features the accuracy and repeatability needed to eliminate processing variability from critical experiments. Recipes are easily entered, monitored, and stored with the convenient full-color touch screen interface and onboard DataStream™ Technology. Compact footprint, intuitive design, and unparalleled manufacturer experience add up to years of high-performance bake step processing, perfect for any low-volume or R&D laboratory processing environment.

### 2.1 User Controls

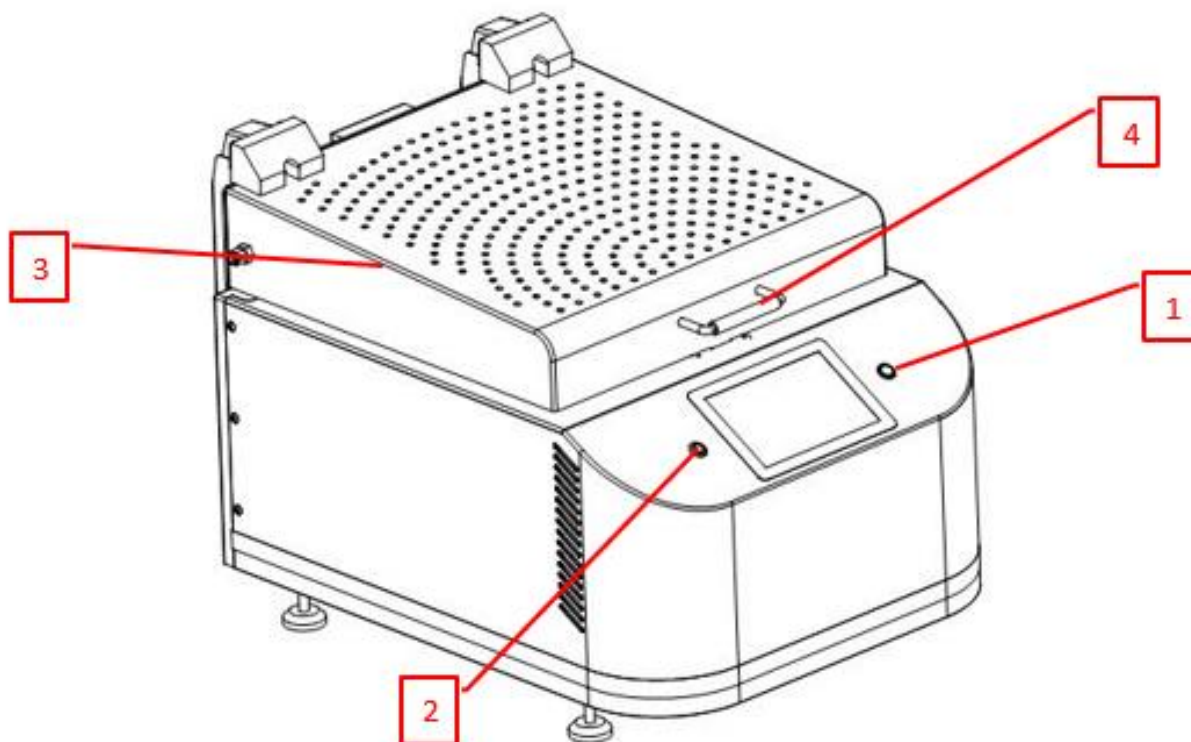


Figure 1: Cee® Apogee® 300 Bake Plate User Controls

1. power button .....used to turn equipment off and on
2. user presence button<sup>1</sup> ..... facilitates remote access
3. bake plate lid .....cover for the bake plate working surface
4. lid handle .....enables safe opening and closing of the lid

### 2.2 Dimensions

- 18.75" (477mm) W x 26.25" (667mm) D x 17.75" (451mm) H
- machine weight..... 146lbs (66.2kg) *excluding accessories*

<sup>1</sup> See [DataStream™ Manual](#) for more information

## 2.3 Features & Programmability

- compact design for minimized footprint
- 7" touch screen display with full-color alphanumeric-capable graphical user interface (GUI)
- durable wet bench design can be converted to a flange/deck mountable configuration
- supports unlimited bake process programs/program steps per recipe
- 0.1 second step time resolution (9,999.9 seconds maximum step time)
- three automated bake methods: contact, vacuum, proximity (N<sub>2</sub> or lift pins)
- bake plate auto-sizing for 100mm, 125mm, 150mm, 200mm and 300mm substrates<sup>2</sup>
- up/download DataStream™ process parameters via native USB and Ethernet ports
- program 10 specific proximity heights above surface in any sequence/combination
- height programmed in 0.1 increments with an overall range of 0-19mm
- exhausted hood for removal of process chemicals
- optional nitrogen purge for inert bake environment

## 2.4 Precision

- substrate sizes..... <10mm to 300mm round; 12" x 12" square
- temperature resolution ..... 0.1°C
- temperature range..... ambient to 300°C (400°C optional)
- temperature uniformity ..... ± 0.3% across working surface


## 2.5 Reliability

- industry-leading Cee® Apogee® reliability and uptime
- one-year full warranty on parts and labor
- complimentary remote technical support and application process assistance for the life of the product

## 2.6 NRTL

Beginning in June of 2024, all standard Cee® Apogee® 300 Bake Plate models will proudly showcase the TÜV SÜD NRTL mark, a testament to our commitment to safety and quality.

The TÜV SÜD NRTL mark signifies compliance with North American safety standards, providing assurance of product safety and quality. Recognized by Authorities Having Jurisdiction (AHJs) and code officials throughout the US and Canada, the TÜV SÜD Mark is featured on millions of products sold nationwide. Customers can trust that products bearing the TÜV SÜD Mark meet rigorous safety standards established by independent testing and ongoing inspections.

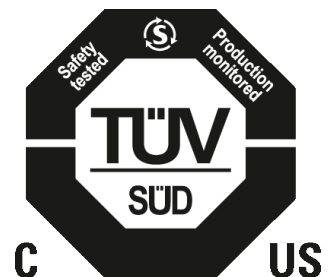

---

<sup>2</sup> Equipment may allow for custom sized substrates based on customer request.

## 2.7 Utilities

- voltage ranges..... 208-230 VAC, single phase 50/60 Hz
- power requirements ..... 3744W (16.3A) *max*
- exhaust port..... 2" OD, 0.4" H<sub>2</sub>O@10CFM (100Pa@17 CMH)
- vacuum..... 20 inHg (33kPa abs)
- N<sub>2</sub>..... 35psi (241kPa)

3 **Installation**

3.1 **Clearance Requirements**

The Cee® Apogee® 300 Bake Plate is a benchtop unit requiring a table or benchtop for location. In most cases the supporting structure will be larger than the unit itself.


**Clearance Requirements**

Adherence to these requirements ensures adequate spacing, ventilation, and access to the detachable MAINS<sup>3</sup> supply cords as needed.

device rear ..... 12" (304.8mm)  
device sides ..... 3" (76.2mm)



Figure 2: Apogee® 300 Bake Plate Side Clearance Requirements

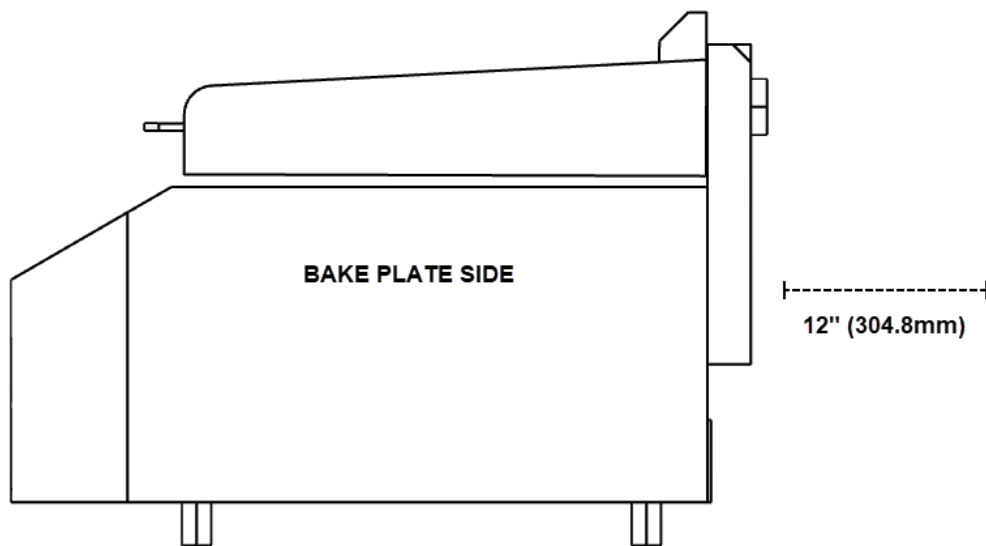

<sup>3</sup> The tool should only be operated with the MAINS supply cord provided by Cee®.

Figure 3: Apogee® 300 Bake Plate Rear Clearance Requirements

### 3.2 Facilities Requirements

The Cee® Apogee® 300 Bake Plate requires the following utilities for operation.

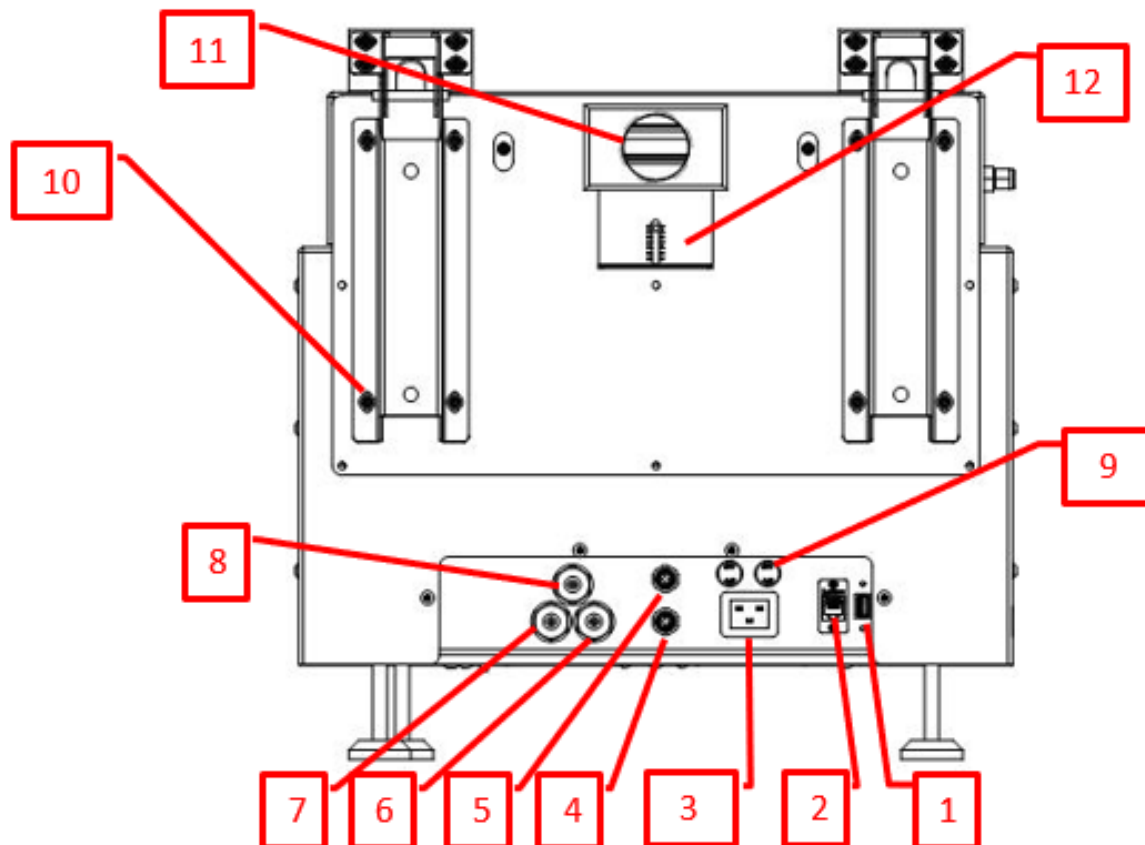


Figure 4: Apogee® 300 Bake Plate Facilities Connections

1. USB port ..... facilitates data transfer
2. Ethernet ..... enables remote recipe writing remote device control
3. AC power in..... single phase 208-230 VAC at 16.3A
4. accessory port..... as needed, M12 4pin, male, 24VDC
5. light tree..... (optional) light tree port, M12 4pin, female, 24VDC
6. vacuum accessory supply..... (optional) 1/4" NPT port
7. system vacuum ..... 1/4" NPT port, <33kPa abs
8. system N<sub>2</sub> ..... (optional) system nitrogen/CDA 40psi (275 kPa)
9. fuses ..... system protection fuses (Replacement: BK/MDA-20-R – 20A; 250VAC max)
10. hood height adjustment ..... used to adjust the gap beneath the hood
11. exhaust port..... exhaust port for bake plate vapors
12. exhaust gate..... used to adjust the flow rate of exhaust on the bake plate

### 3.3 Environment

The Cee® Apogee® 300 Bake Plate should be operated in a clean, low humidity environment.

### 3.4 Unpackaging & Inspection

1. Lifting from the bottom of the unit, carefully remove from packing crate. Do not lift by any of the top covers or protrusions. Do not roll or turn the unit on its sides.
2. Remove packing foam and plastic wrap.
3. Place the Cee® Apogee® 300 Bake Plate on a table of proper height and strength so that the controls and bake surface are at an ergonomically appropriate height.
4. Thoroughly check the machine for shipping damage. If physical damage is apparent, ***DO NOT APPLY POWER!*** Contact [Cee® Customer Support](#) immediately.

*\*All Apogee® Bake surface plates are Type III anodized aluminum and conform to industry specifications for hardness and durability. Please note that the color of the surface plates may vary due to the anodizing process. This variance in color does not affect the quality, functionality, or performance of the product.*

#### **The following items are included with shipment:**

- Cee® Apogee® Bake Plate
- (x2) stop pins
- temperature & humidity sensor
- power cord
- operations manual (USB thumb drive)
- quick reference card

#### **Optionally Included Items:**

- vacuum pump
- other equipment as specified by your sales order

### 3.5 System Installation & Setup

Please refer to the quick reference card supplied with the tool.

1. Using (x2) 9/16" wrenches, turn the adjustable feet until there is 1 ¼" – 1 ¾" between the tabletop and bottom of the equipment. Using the adjustable feet, first level the Cee® Apogee® Bake Plate then adjust so that the bake surface tilts slightly back sufficiently that when using *proximity mode* the wafer floats against the stop pins and not off the front of the chuck.
2. Thoroughly clean the bake plate surface according to instructions outlined in the *Preventative Maintenance* section of this manual.
3. Connect utilities according to the *Facilities Requirements* diagram in section 3.2.
4. Connect the temperature & humidity sensor to the CAN terminal.
5. Connect the vacuum supply to the vacuum fitting.
6. Connect the nitrogen supply to the nitrogen fitting.
7. Connect exhaust lines to the exhaust port.
8. Plug in the machine using the supplied Cee® shielded cables and note that only the cooling fan should be powered, not the display.

### 3.6 Start Up

Once the preliminary setup steps outlined in section 3 have been completed, press the lighted *Power* switch to turn the tool on. The display will cycle through a series of boot screens before arriving at the main login screen.

Enter default administrative login credentials:

**Username:** ..... admin

**Password:** ..... admin2

### 3.7 System Checks

On the **Process** screen, navigate to **Tools>Manual Control** and perform the following system checks for initial validation of the Cee® Apogee® 300 Bake Plate.

#### Set Lift Pins

Select a **Control** of **Lift Pins** and an **Action** of **Set**. Enter a value into the **Height** field and tap **Apply**. Verify **Lift Pin Height** readings respond to changes on the **System Values** list.

Apogee Bake Process Recipes About Tools - admin

Parameter	Actual	Set Point
Plate Temperature	26.2 °C	--
Lift Pin Height	0.0 mm	0.0 mm
Bake Method	Contact	Contact
Ambient Temperature	27.2 °C	
Humidity	45.2 %	

System Controls

Control: Lift Pins

Action: Set

Height: 0 mm

Set lift pins to 0 mm

APPLY

Inset supplied stop pins into the desired holes on the bake plate surface. These stop pins keep the substrate centered on the bake plate surface. Holes closest to center are for 100mm substrates. From center, stop pin locations are for 100mm, 125mm, 150mm, 200mm, 300mm substrates respectively.

#### Bake Methods

##### **Vacuum**

Set **Bake Method** to **Vacuum**. Place a substrate on the center of the bake plate and check that the vacuum holds the substrate.

Apogee Bake Process Recipes About Tools - admin

Parameter	Actual	Set Point
Plate Temperature	26.1 °C	--
Lift Pin Height	0.0 mm	0.0 mm
Bake Method	Vacuum	Vacuum
Ambient Temperature	27.2 °C	
Humidity	43.5 %	

System Controls

Control: Bake Method

Action: Select Method

Method: Vacuum

Bake using Vacuum method

APPLY

## Proximity

Set **Bake Method** to **Proximity**. This will turn off the vacuum and purge N<sub>2</sub> to float the substrate above the bake plate surface.

The screenshot shows the 'Apogee Bake' interface with the 'Tools' tab selected. On the left, the 'System Values' table lists parameters: Plate Temperature (26.1 °C), Lift Pin Height (0.0 mm), Bake Method (Proximity), Ambient Temperature (27.1 °C), and Humidity (43.0 %). The 'Bake Method' row is highlighted in yellow. On the right, the 'System Controls' panel shows the 'Control' dropdown set to 'Bake Method', the 'Action' dropdown set to 'Select Method', and the 'Method' dropdown set to 'Proximity'. Below these, a button labeled 'Bake using Proximity method' is visible, and at the bottom is a large blue 'APPLY' button. Red boxes highlight the 'Bake Method' dropdown, the 'Proximity' method selection, and the 'APPLY' button, with lines connecting them to show the configuration path.

Parameter	Actual	Set Point
Plate Temperature	26.1 °C	--
Lift Pin Height	0.0 mm	0.0 mm
Bake Method	Proximity	Proximity
Ambient Temperature	27.1 °C	
Humidity	43.0 %	

System Controls

Control: Bake Method

Action: Select Method

Method: Proximity

Bake using Proximity method

APPLY

## Contact

Set the **Bake Method** to **Contact**. This will turn off vacuum and N<sub>2</sub>. Remove the substrate.

The screenshot shows the 'Apogee Bake' interface with the 'Tools' tab selected. On the left, the 'System Values' table lists parameters: Plate Temperature (26.1 °C), Lift Pin Height (0.0 mm), Bake Method (Contact), Ambient Temperature (27.2 °C), and Humidity (43.3 %). The 'Bake Method' row is highlighted in yellow. On the right, the 'System Controls' panel shows the 'Control' dropdown set to 'Bake Method', the 'Action' dropdown set to 'Select Method', and the 'Method' dropdown set to 'Contact'. Below these, a button labeled 'Bake using Contact method' is visible, and at the bottom is a large blue 'APPLY' button. Red boxes highlight the 'Bake Method' dropdown, the 'Contact' method selection, and the 'APPLY' button, with lines connecting them to show the configuration path.

Parameter	Actual	Set Point
Plate Temperature	26.1 °C	--
Lift Pin Height	0.0 mm	0.0 mm
Bake Method	Contact	Contact
Ambient Temperature	27.2 °C	
Humidity	43.3 %	

System Controls

Control: Bake Method

Action: Select Method

Method: Contact

Bake using Contact method

APPLY

## Temperature & Humidity Sensor

Ensure the temperature & humidity sensor is functioning by verifying that **Ambient Temperature** and **Humidity** readings are present on the **System Values** List.

The screenshot shows the 'Apogee Bake' interface with the 'Tools' tab selected. On the left, the 'System Values' table lists parameters: Plate Temperature (24.4 °C), Lift Pin Height (19.0 mm), Bake Method (Contact), Ambient Temperature (25.2 °C), Humidity (45.1 %), and Empty Sensor (False). The 'Ambient Temperature' and 'Humidity' rows are highlighted in yellow. On the right, the 'System Controls' panel shows the 'Control' dropdown set to 'Bake Method', the 'Action' dropdown set to 'Select Method', and the 'Method' dropdown set to 'Contact'. Below these, a button labeled 'Bake using Contact method' is visible, and at the bottom is a large blue 'APPLY' button.

Parameter	Actual	Set Point
Plate Temperature	24.4 °C	--
Lift Pin Height	19.0 mm	19.0 mm
Bake Method	Contact	Contact
Ambient Temperature	25.2 °C	
Humidity	45.1 %	
Empty Sensor	False	

System Controls

Control: Bake Method

Action: Select Method

Method: Contact

Bake using Contact method

APPLY

## Enable & Test Plate Temperature

Use the **Control** drop-down to select **Plate Temperature** then select an **Action** of **Set**, enter the desired plate temperature for your application, and tap **Apply**. \*Note that the **System Values** list displays a Set Point of null (--).



Apogee Bake Process Recipes About **Tools** admin

System Values

Parameter	Actual	Set Point
Plate Temperature	26.2 °C	--
Lift Pin Height	0.0 mm	0.0 mm
Bake Method	Contact	Contact
Ambient Temperature	27.2 °C	
Humidity	43.4 %	

System Controls

Control 

Plate Temperature

Action 

Set

Value 

90

 °C

Set temperature to 90 °C

APPLY

Change the **Control** selection to **Plate Temperature** then select **Enable** from the **Action** and **Value** dropdowns and tap **Apply**. Note that the temperature entered in the previous step is now displayed as the **Set Point** in the *System Values* list. The **Actual** temperature in the *System Values* list will increase/decrease as the bake surface heats/cools.

Apogee Bake Process Recipes About **Tools** admin

System Values

Parameter	Actual	Set Point
Plate Temperature	27.5 °C	90.0 °C
Lift Pin Height	0.0 mm	0.0 mm
Bake Method	Contact	Contact
Ambient Temperature	27.2 °C	
Humidity	43.2 %	

System Controls

Control 

Plate Temperature

Action 

Enable

Value 

Enable

Enable temperature controller

APPLY

Once these operations have been validated, the Cee® Apogee® 300 Bake Plate is ready for use. Begin by creating a recipe. Refer to the [DataStream™ Manual](#) for more information and refer to section 4 of this manual for Bake Plate specific DataStream™ features.

***\*In the event of a fault condition, power cycle the tool to restore function***

## 4 DataStream™ Technology

This section covers information specific to the Apogee® 300 Bake Plate and is intended as a companion to the DataStream™ Technology Software Manual. **Please review the DataStream™ Operations Manual** for detailed guidance on software usage.

### 4.1 System Parameters

Parameter	Actual	Set Point	Status
Plate Temperature	59.4 °C	60.0 °C	In Range
Lift Pin Height	19.0 mm	19.0 mm	In Range
Bake Method	Contact	Contact	In Range
Ambient Temperature	26.5 °C		In Range
Humidity	44.8 %		In Range

#### Plate Temperature<sup>4</sup>

the current temperature of the hot chuck displayed against the target set point in degrees Celsius

#### Lift Pin Height

the height of exposed lift pins in relation to the chuck in millimeters; precision control settings range from 0.0-19.0

#### Bake Method

dictates the manner in which the substrate is heated; vacuum, contact, proximity, lift pins.

#### Ambient Temperature

the air temperature of the environment where the equipment is housed

#### Humidity<sup>5</sup>

the ambient relative humidity in the environment where the equipment is housed

### 4.2 Manual Controls – Apogee® 300 Bake Plate

The **Manual Control** activity is an advanced feature that allows users to run most operating processes outside of a recipe. This mode is useful for tasks such as prototyping processes, verifying equipment operation, and recovering from aborted processes. To access the activity, navigate to **Tools > Manual Control**. Actual and set point parameter values are displayed on the left. Available controls will be selected from the dropdown menu on the right.

*If using remote feature, the user must confirm local presence to execute manual commands. Refer to the [DataStream™ Manual](#) for guidance on the Local Presence feature.*

The screenshot shows the Apogee Bake software interface. On the left, under 'System Values', there is a table with columns 'Parameter', 'Actual', and 'Set Point'. The table lists: Plate Temperature (24.5 °C, --), Lift Pin Height (19.0 mm, 19.0 mm), Bake Method (Contact, Contact), Ambient Temperature (26.7 °C), and Humidity (41.4 %). On the right, under 'System Controls', there is a 'Control' dropdown menu with the text 'What do you want to control?' and a list of options: Plate Temperature, Lift Pins, and Bake Method. Below the dropdown is a button labeled 'APPLY'.

<sup>4</sup> A process will not wait to achieve desired temperatures before moving onto the next step. Utilize preconditions or manual controls to ensure platen temperatures are in range before a process is initiated.

<sup>5</sup> Both Ambient Temperature and Humidity are measured via a custom sensor board mounted next to a ventilation inlet inside the tool. If sensor is disconnected, default of -1.1 is displayed.

## Plate Temperature

System Values		
Parameter	Actual	Set Point
Plate Temperature	41.5 °C	--
Lift Pin Height	-1.0 mm	5.0 mm
Bake Method	Contact	Contact
Ambient Temperature	25.1 °C	
Humidity	45.5 %	

System Controls	
Control	Plate Temperature
Action	Set
Value	45 °C
Please check your values before applying the change.	

Select a Control of Plate Temperature  
Select an Action of Set  
Enter the desired value in °C

**Click APPLY**

The Temperature Controller must be enabled to initiate the heating process. See next step.

System Values		
Parameter	Actual	Set Point
Plate Temperature	41.9 °C	45.0 °C
Lift Pin Height	-1.0 mm	5.0 mm
Bake Method	Contact	Contact
Ambient Temperature	25.0 °C	
Humidity	44.4 %	

System Controls	
Control	Plate Temperature
Action	Enable
Value	Enable
Enable temperature controller	

Select an Action of Enable  
Select a Value of Enable or Disable to activate or deactivate the temperature controller

**Click APPLY**

Note that the heating process has been initiated and a plate temperature set point has populated on the system values list. When a value of Disabled is selected, a Set Point of - - is displayed and the heating process is terminated.

System Controls	
Control	Plate Temperature
Action	AutoTune

Select an Action of AutoTune

**Click APPLY**

User must first define the set point and enable temperature controller.

Useful for refining the temperature control for a given setting – note that this may take a significant amount of time.

**System Controls**

**Control** Plate Temperature

**Action** Ramp

**Target** 30 °C

**Rate** 2 °C / Minute

Select an Action of *Ramp*

Enter the Target temperature

Enter the desired ramp Rate<sup>6</sup> (between 1-6°C per minute)

**Click APPLY**

### Lift Pins

**System Values**

Parameter	Actual	Set Point
Plate Temperature	42.9 °C	45.0 °C
Lift Pin Height	10.0 mm	10.0 mm
Bake Method	Contact	Contact
Ambient Temperature	25.0 °C	
Humidity	44.7 %	

**System Controls**

**Control** Lift Pins

**Action** Set

**Height** 10 mm

Set lift pins to 10 mm

Select a Control of *Lift Pins*

Select an Action of *Set*

Enter the target height (between 0-19mm)

**Click APPLY**

Note that the lift pin height set point has populated on the system values list.

<sup>6</sup> Cee® does not offer active cooling on bake plates however, the ramp feature can be used to reduce the rate of cooling beyond what ambient conditions allow.

System Controls

Control

Lift Pins

Action

Go Home

Select an Action of *Go Home*

**Click APPLY**

Lift pins recede beneath the surface of the hot plate until they contact the homing flag for recalibration of position.

System Controls

Control

Lift Pins

Action

Step

Step Size

19

mm

Direction

Up

Select an Action of *Step*

Enter the desired Step Size (between 0-19mm)

Select the preferred Direction

**Click APPLY**

System Controls

Control

Lift Pins

Action

Raise Pins

Select an Action of *Raise Lift Pins*

**Click APPLY**

Set pins to the Lift Pin Idle Position specified in section 4.6 **Tool Specific Settings – Apogee® 300 Bake Plate**. Review the [Apogee® 300 Bake Plate Operations Manual](#) for more information.

System Controls

Control
Lift Pins

Action
Lower Pins

Select an Action of *Lower Lift Pins*

**Click APPLY**

Lift pins recede just beneath the surface of the hot plate to facilitate contact with the substrate.

### Bake Method

System Values

Parameter	Actual	Set Point
Plate Temperature	45.3 °C	45.0 °C
Lift Pin Height	10.0 mm	10.0 mm
Bake Method	Contact	Contact
Ambient Temperature	25.1 °C	
Humidity	44.7 %	

System Controls

Control
Bake Method

Action
Select Method

Method
Contact

Bake using Contact method

Select a Control of Bake Method

Select the desired Method (Vacuum, Proximity, or Contact)

**Click APPLY**

Review the [Apogee® 300 Bake Plate Operations Manual](#) for more information on Bake Methods.

### 4.3 Preparation

Users with sufficient privileges can **Prepare** equipment to run a recipe. This feature is useful for preconditions and parameters that take a significant amount of time such as hot chuck and platen temperatures. To initiate this feature, navigate to the **Recipes** tab, click **Load** to access the recipes list and select the desired recipe, then click **Prepare**.

Apogee Bake Process **Recipes** About Tools - admin

Recipe Controls

Load

**Prepare**

Run

New

Viewing Recipe- Test\_Red\_Recipe

Name Test\_Red\_Recipe Notes

Plate Temperature 180 °C

Step Time (seconds) Process Method Pin Height (mm)

1 60 Contact

**\*Preparation processes cannot be initiated when the equipment is already in use.**

**Local Display** – When a **Prepare** command is entered, the user or device with active control of the machine receives an alert. This prompt includes the user and recipe to be prepared. The user with control of the machine can refuse the request by selecting **Abort** or accept the request by tapping **OK**.

In the absence of a response, the request is auto accepted after two minutes.

User (admin) attempting to set temperature for recipe:

Test\_Red\_Recipe

Press OK to continue or ABORT to cancel.

OK

00:00:01

Recipe Preparation Abort

**Preparation In Process** – progress toward the specified precondition(s) is displayed to the user with verified local presence.

Apogee Bake **Process** Recipes About Tools - admin


! Plate Temperature( 130.0 °C ) - Within -5% and +5% of 180 °C

Waiting on preconditions to be in range for recipe ...

(PREHEAT) - Test\_Red\_Recipe

100% Elapsed 00:00:18 ABORT Remaining 00:00:00


**Preparation Complete** – indicates that the equipment has reached all specified preconditions and the recipe can be initiated. Upon clicking **OK** the user is directed to the *Process* screen to begin the recipe.

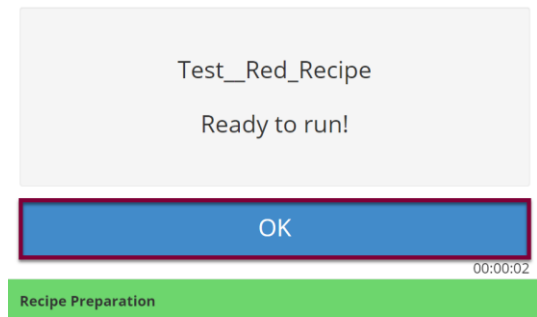


*\*During recipe preparation the Prepare and Run commands are disabled to ensure no interruption to precondition processes.*

#### 4.4 Running Recipes


1. Select Recipe Page



2. Load Recipe

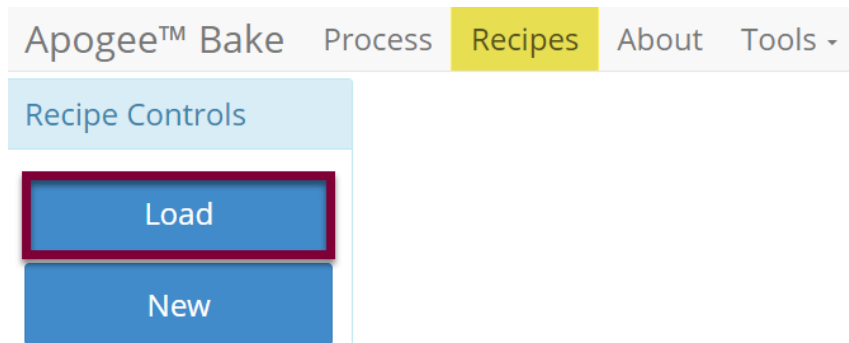

3. Search For, Identify, & Select Recipe

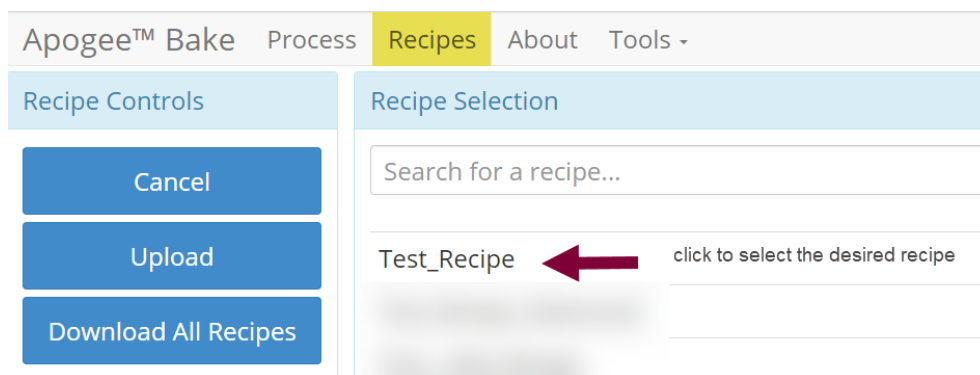

4. Run Recipe



Apogee™ Bake
Process
**Recipes**
About
Tools -

Recipe Controls

Load
Run

Viewing Recipe- Test\_Recipe

Name
Test\_Recipe

Notes

## 5. Start Recipe

Apogee™ Bake
**Process**
Recipes
About
Tools -
admin

Test\_Recipe : Recipe Progress

1		Load Wafer	
2		Enable temperature controller	
3		Set temperature to 35 °C	
4		Start iteration	
5		Set lift pins to 4 mm	

Step 1 of 10
Iteration 1 of 4

100%

Elapsed  
00:00:00

START

Remaining  
00:00:00

## 6. Recipe Progression

Step 7 of 10
Iteration 1 of 4

0%

Elapsed  
00:00:05

ABORT

Remaining  
00:05:00

\*Users may be required to follow prompts on the screen during recipe execution.

## 4.5 Editing Recipes

Apogee™ Bake
Process
**Recipes**
About
Tools -
admin

Editor Controls

Save
Cancel
Insert
^
v
Delete
Advanced

Editing Recipe- Test\_Recipe

Name
Test\_Recipe

Plate Temperature
120
°C

Notes

Step	Time (seconds)	Process Method	Pin Height (mm)
1	60	Contact	
2	30	Contact	
3	30	Contact	
4	60	Proximity	

#### 4.6 Tool Specific Settings – Apogee® 300 Bake Plate

<b>Temperature Offset Calibration (°C)</b>	Offset used by the temperature controller to calibrate the reported chuck temperature
<b>Lift Pin Idle Position (mm)</b>	User defined height of lift pins upon machine start-up and after recipe completion *default value 19mm
<b>Lift Pin Offset (mm)<sup>7</sup></b>	Offset can be supplied for calibration of lift pin positioning

---

<sup>7</sup> Offset impacts all lift pins.

## 5 Bake Plate Theory

Hotplate bake processing has increased in popularity since the early 1980s. Previously the most common technique for film drying and curing was the convection oven. Bake plates, also known as hotplates, offer several advantages in the form of increased throughput, increased uniformity and reproducibility, and decreased particle contamination. In a typical bake process, the substrate quickly rises to temperature. Drying and curing steps generally take about one minute. This contrasts with traditional oven processes which generally take thirty minutes or more.

### 5.1 Bake Plates vs Conventional Ovens

Bake plates have several advantages over conventional ovens.

- decreased bake time
- increased reproducibility
- better film quality

This section will describe these differences and set a few guidelines for using bake plates.

Stratification, the formation of different temperature zones, is a problem associated with convection ovens and can severely affect film quality and reproducibility.

The heating rate of a substrate in an oven depends not only on the heated air flow past a substrate but also on its proximity to other cold substrates. Thus, the heating rate for each substrate in a cassette of substrates that are being baked will be less than if each substrate is baked alone.

In addition, substrates near the ends of a cassette heat faster than the substrates in the middle, producing a non-uniform heating.




Particle generation also occurs within a standard oven. In a forced-air convection oven, substrates are commonly exposed to a flow of particle laden air for at least thirty minutes.

During resin film cures, the substrates will be exposed to considerable particulate contamination. The substrates are vulnerable since the film may still contain solvents and during this *soft* state the film is very susceptible to having particle adhere to it.

### 5.2 The Skin Effect

Another disadvantage of normal oven baking results from baking substrates from the *outside in*. Since heat is applied to the outer surface of the film first, a skin forms on the surface of the film, trapping solvents. Upon vaporizing, these solvents form blisters or bubbles which results in adhesion loss or even bulk film failure. This problem prevails in processes involving thick film resins, e.g., polyimides.

No skin effect occurs on a hotplate since hotplate baking heats the substrate from the bottom up. This *inside out* approach offers advantages for thick films since solvents in the film nearest the substrate are baked off before the film surface seals over.

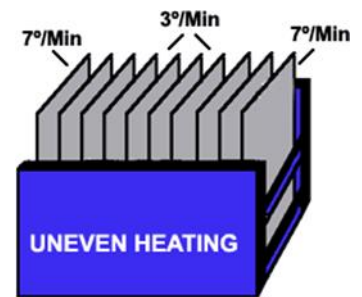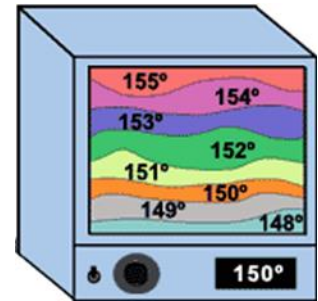

### 5.3 Hotplate Bake Variables and Methods

A typical bake process consists of preheating the surface to a known temperature, loading the substrate onto the surface for a specific length of time and removing it promptly at the end of the cycle. The selection of the temperature and time values used as well as the bake method employed all affect the overall performance of the process.


### 5.4 Bake Temperature

The bake temperature used is dependent on several factors. The material and substrate being baked as well as the results desired are key factors to be considered in developing a bake process

In general, hotplate baking will be performed at temperatures slightly higher than those used in oven bake processes. The film being baked will reach a temperature somewhere between the temperature of the hotplate and the ambient air above the film. As an example, with a hotplate surface temperature of 115°C, a layer of photoresist on a silicon wafer will reach a final temperature of about 105°C after a few seconds. Thicker substrates and/or substrates with lower coefficients of thermal conductivity will require even higher temperatures to compensate for this phenomenon.

### 5.5 Bake Methods

Another important factor is the method of bake. Cee® hotplates allow for three distinct bake methods:

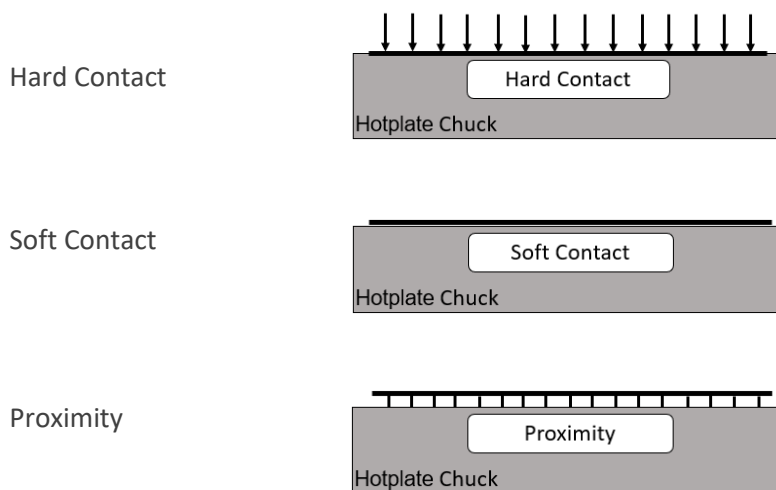

In a hard contact bake, the substrate is held onto the hotplate surface by the application of vacuum to the underside of the substrate. Small holes are machined into the hotplate surface in a pattern which optimizes vacuum distribution without the formation of cold spots or warping of the substrate. This method is usually preferred for silicon and other flat substrates where back side contact is not a problem.

Soft contact baking uses gravity alone to hold the substrate to the hotplate. This method generally offers less uniformity since the substrate-hotplate thermal interface is not as efficient.

Proximity baking is accomplished by forcing nitrogen through ports in the hotplate surface. This forces the substrate to float at a distance of one to four millimeters (25-100µm) above the hotplate surface. Proximity baking allows for a slower warm-up than contact bake methods and can be advantageous when baking thick films where blistering would otherwise be a problem.


Another advantage of proximity baking is that often, cambered, or warped substrates can be baked with a high degree of uniformity. This is usually not possible with the contact methods since it is not possible to achieve a vacuum under a substrate that is not flat to start with. Processing cambered substrates with the soft contact

method creates hot spots where the substrate touches the hotplate and cold spots where it does not. It should be noted as well that this type of proximity process is *self-leveling* in that substrate will tend form a uniform gap to the hotplate surface.


Proximity baking also offers the unique advantage of allowing hotplate processing without touching the bottom side of the substrate. An example of this application is photomask processing. In processing these relatively thick glass plates it is important that the backside of the glass not directly touch the hotplate since rapid heating will cause micro-fractures in the glass. By performing the entire bake process in proximity mode, the integrity of the substrate is not endangered, and the uniformity is excellent.

## 5.6 Bake Time

The selection of the bake time parameter plays an important role in the reproducibility of the bake process. Substrate thermal properties and the choice of bake method greatly affect the amount of time necessary for the substrate, and therefore film temperature, to stabilize during the bake. Thicker substrates and the use of proximity bake methods will increase the time necessary for the film to reach its final temperature. It is important that most of the baking action in the film take place after this temperature is reached. A silicon wafer will reach a stable temperature within a few seconds and so it is traditional to adjust photoresist bake processes to be completed in 60-90 seconds with an appropriate bake temperature.

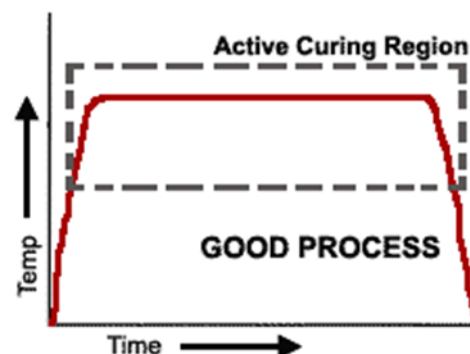


For thicker substrates such as photomask and ceramic modules, the increased time necessary to heat the larger mass of the substrate results in bake times approaching five minutes. It should be noted that these substrates can be processed with higher temperature and shorter bake times, but reproducibility may suffer. If the bake time is too short, a significant amount of the actual bake process will take place during the loading and unloading steps as well as while the substrate is cooling after removal from the bake plate. This is an unstable condition since it is very difficult to exactly reproduce conditions during these steps.

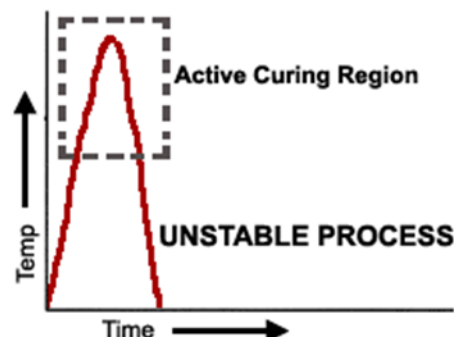

In general, the temperature-time relationship in a bake process can be taken as a dose of the (temperature) x (time) product. Increasing the bake temperature results in a need for decreasing bake time. The limits for both parameters can be reached when the process is no longer reproducible or when the physical temperature limitations of the resin or substrate have been reached.

## 5.7 Exhaust Cover

The design of the Cee® exhaust cover promotes dissipation of vapors removed from a substrate placed on the chuck, without drawing air across the chuck surface.

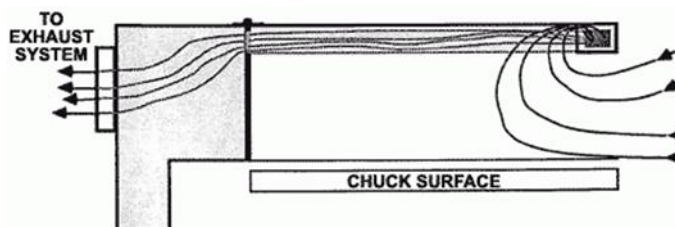

## 5.8 Oven vs Bake Plate Examples

The chart below presents process examples for commonly used resins. These figures should not be used as a rigid guideline since the best method with a particular baking application can only be achieved through experimentation.

## **Application**

Positive Photo Resist

## **Oven Bake**

90°C, 30 minutes, Polyimide beta (partial imidization)

135°C, 30 minutes, Polyimide alpha (solvent removal)


## **Hotplate Bake**

115°C, 30 seconds, hard contact bake, Polyimide beta (partial imidization)

150°C, 15 seconds, proximity bake, 150°C-90 seconds, hard contact bake, Polyimide alpha (solvent removal)

## **5.9 Reflow Soldering**

Bake plate processing heats the substrate and the solder without applying heat directly to the devices on the board. Using a combination of proximity and hard-contact bakes, the bake profile can be adjusted to suit any process.

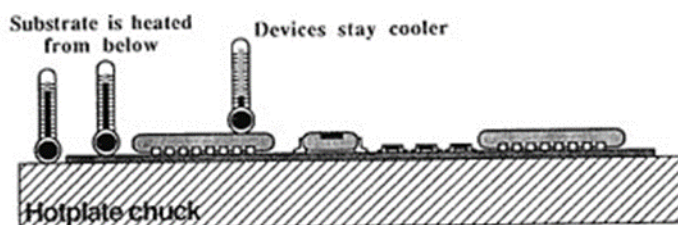

## **5.10 Bake Plate Process Troubleshooting**

As with spin coating process, there are no absolute rules for bake plate processing, only general guidelines. The following is a list of issues to consider for specific bake plate process problems.

### **Film overbaked**

bake temperature too high.....reduce temperature

bake time too long .....decrease bake time

### **Film underbaked**

bake temperature too low .....increase temperature

bake time too short .....increase bake time

### **Film blistering or cracking**

unstable balance in temp/time parameters .....decrease temp/increase time

warm-up time too fast .....use proximity bake to preheat substrate

### **Non-uniform bake**

unstable balance in temp/time parameters .....decrease temp/increase time

operating with exhaust lid raised .....lower the exhaust lid

unstable ambient conditions .....protect against major fluctuations

bake time too short .....increase bake time





bake plate surface contaminated .....clean surface of bake plate

## 6 Preventative Maintenance

This section provides personnel with procedures and guidelines for maintaining a Cee® Apogee® Bake Plate.

### 6.1 Service and Repairs

#### **Safety Notice: Important Repair Information for Cee® Equipment**

	In order to maintain safety and performance standards, only authorized representatives of Cee® are permitted to conduct repairs or alterations on Cee® equipment.	Afin de maintenir les normes de sécurité et de performance, seuls les représentants autorisés de Cee® sont autorisés à effectuer des réparations ou des modifications sur l'équipement Cee®.
	When servicing the machine, use only replacement parts made or recommended by Cee®.	Lors de l'entretien de la machine, utilisez uniquement des pièces de rechange fabriquées ou recommandées par Cee®.
	Use only Cee® supplied shielded cables with this machine.	Utilisez uniquement les câbles blindés fournis par Cee® avec cette machine.
	Unauthorized repairs may lead to serious risks such as equipment malfunction, damage, personal injury, or even death.	Les réparations non autorisées peuvent entraîner des risques graves tels qu'un dysfonctionnement de l'équipement, des dommages, des blessures corporelles, voire la mort.

### 6.2 Fault Condition

In the event of a fault condition, power cycle the tool to restore function.

### 6.3 Safety Checks

Inspect bake plate lid for the following defects:

- loose assemblies
- improper closure
- improper exhaust connection

### 6.4 Mechanical/Utilities Checklist

<u>Evaluate</u>	<u>Frequency</u>	<u>Detail</u>
Utility Gasses & Vacuum	Daily	Check all gas pressures and vacuum for ranges specified in tool manual.

<b>Exhaust</b>	Daily	Verify that the exhaust is functional with adequate flow.
<b>Bake Plate Surface</b>	Weekly	Buildup of material on the bake plate can cause vacuum errors. For minor build-up wipe the bake surface clean with isopropyl alcohol or acetone. For major build-up of material, utilize a glass slide held at a 45° angle to <b><i>gently</i></b> scrape the material away then wipe clean with isopropyl alcohol or acetone.
<b>Lift Pin Height</b>	Quarterly	If the three lift pins are not lifting the wafer programmed amount of distance from the bake plate surface, they may require calibration. See section 4.6 <b>Tool Specific Settings – Apogee® 300 Bake Plate</b> for details.
<b>Power</b>	Bi-Annually	Verify that AC power is connected and of the proper voltage.

## 6.5 Cleaning

The Apogee® 300 Bake Plate should be cleaned following daily use and only after the equipment has cooled to a safe thermal condition. The cabinet should be cleaned with isopropyl alcohol. When cleaning the hot plate surface, it is good practice to use the mildest solvent possible such as acetone or isopropyl alcohol. ***Do not use caustic acids or bases.*** For major build-up of material, utilize a glass slide held at a 45° angle to gently scrape the material away then wipe clean with isopropyl alcohol or acetone. Please visit the Cee® YouTube Channel for a [demonstration](#). If these methods are unsuccessful contact [Cee® Customer Support](#) for additional guidance.

Use only water-based cleaner on the labels on the rear of the machine. Use only isopropyl or water- based cleaner on the Power, Cee® logo, Caution ... Eye Protection, and the Cee® model/serial number labels. The display may be cleaned with glass cleaner, water, or isopropyl alcohol.



## 7 Table of Revisions

Doc Rev #	Author	Description of Change(s)	Reviewed/Approved By	Date
2.4	J. Adams	<ul style="list-style-type: none"> <li>- Update Section 3.4 Unpackaging &amp; Inspection with Type III hard coat information.</li> </ul>	B. Waterworth	12/09/2024
2.3	J. Adams	<ul style="list-style-type: none"> <li>- Add Section 2.6 NRTL</li> </ul>	B. Waterworth	7/11/2024
2.2	J. Adams	<ul style="list-style-type: none"> <li>- Added French translations to all warnings throughout the manual.</li> <li>- Updated Section 1.3 Returned Materials to Include Cee® Physical Address</li> <li>- Updated Section 1.9 Thermal with appropriate warning symbol.</li> <li>- Updated Section 1.10 Chemical with appropriate warning symbol.</li> <li>- Updated voltage ratings to Sections 0</li> <li>- Utilities</li> <li>- and 3.2 Facilities Requirements</li> </ul>	B. Waterworth	6/03/2024
2.1	J. Adams	<ul style="list-style-type: none"> <li>- Update Apogee™ to Apogee®</li> <li>- Amended section 1.12 Intended Use of Machine</li> <li>- Amended section 0</li> <li>- Utilities</li> <li>- Amended section 3.2 Facilities Requirements</li> <li>- Amended section 3.4 Unpackaging &amp; Inspection</li> <li>- Added sections 6.1 &amp; 6.2 to Preventative Maintenance</li> </ul>	B. Waterworth	8/30/2023

2.0	J. Adams	<ul style="list-style-type: none"> <li>- update format</li> <li>- add section 3.1, Clearance Requirements</li> <li>- add section 4, DataStream™ Technology</li> <li>- add section 7, Table of Revisions</li> </ul>	B. Waterworth J. Strothmann	11/09/2022
-----	----------	--	--------------------------------	------------